


Feeding Tube and
Feeding Set

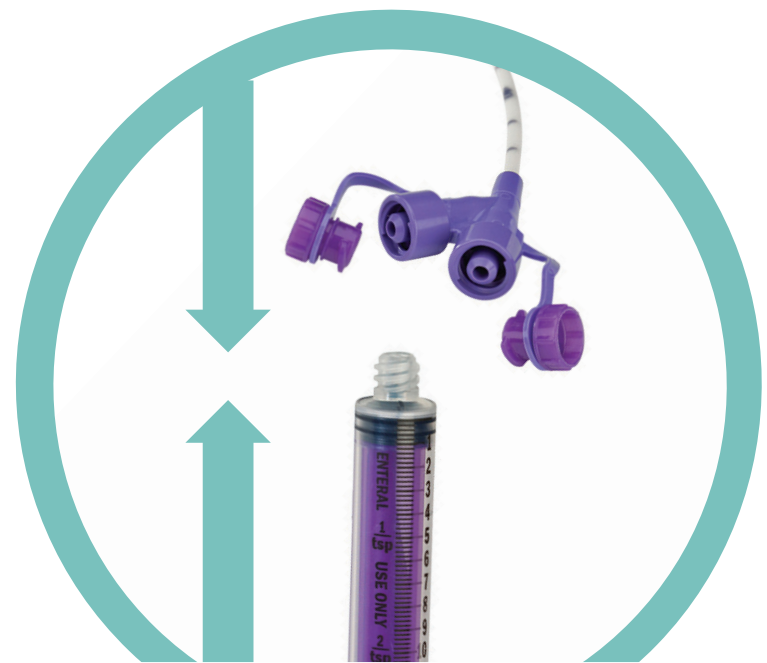

Feeding Tube and
Syringe

Suggested **positioning** for the **connection** of **ENFit™***

Positioning the **feeding tube facing down** upon connection may **prevent formula build-up** in the moat.

Any potential **build-up in the moat** **can cause difficulty** when disconnecting the feeding tube once the formula dries.

Caution:

Do not overtighten the connection.